



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

TECHNICAL DATA SHEET

THUNDER™ Phospho-eIF2 α (S51) + Total eIF2 α TR-FRET Cell Signaling Assay Kit



bioauxilium
BETTER TOOLS. REAL DISCOVERIES.

CATALOG NUMBERS KIT-EIF2APT-500
400 points for phospho-eIF2 α
and 100 points for total eIF2 α

Store at -80°C
For research use only.
Not for use in diagnostic procedures.

PRODUCT DESCRIPTION

This assay kit measures intracellular levels of **phospho-eIF2 α (S51)** and **total eIF2 α** protein in cell lysates using a simple, rapid and sensitive immunoassay based on the homogeneous (no-wash) THUNDER™ TR-FRET technology. The kit is compatible with both adherent and suspension cells.

SPECIFICITY

This assay kit contains two specific and selective antibody pairs, one that recognizes **eIF2 α** phosphorylated at **Ser51** and another that recognizes **total** (both phosphorylated and unphosphorylated) **eIF2 α** .

SPECIES REACTIVITY

Human (Swiss-Prot Acc.: P05198; Entrez-Gene Id: 1965).

Other species should be tested on a case-by-case basis.

TR-FRET ASSAY PRINCIPLE

The **Phospho-eIF2 α (S51) + Total eIF2 α** assay kit is a homogeneous time-resolved Förster resonance energy transfer (TR-FRET) sandwich immunoassay (Figure 1). The THUNDER™ Cell Signaling assay workflow consists of 3 steps (Figure 2). Following cell treatment, cells are first lysed with the specific Lysis Buffer provided in the kit. Then **Phospho-eIF2 α (S51)** and **Total eIF2 α** in the cell lysates are detected in separate wells with two pairs of fluorophore-labeled antibodies in a simple "add-incubate-measure" format (single-step reagent addition; no wash steps). For detection of the phosphorylated protein, one antibody is labeled with a donor fluorophore (Europium chelate; Eu-Ab1) and the second with a far-red acceptor fluorophore (FR-Ab2). The same approach is used for the second antibody pair detecting the total protein (Eu-Ab3 and FR-Ab4). The binding of the two matched labeled antibodies to distinct epitopes on the target protein (either **phospho-eIF2 α** or **total eIF2 α**) takes place in solution and brings the two dyes into close proximity. Excitation of the donor Europium chelate molecules with a flash lamp (320 or 340 nm) or a laser (337 nm) triggers a FRET from the donor to the acceptor molecules, which in turn emit a TR-FRET signal at 665 nm. Residual energy from the Eu chelate generates light at 615 nm. The signal at 665 nm is proportional to the concentration of **Phospho-eIF2 α (S51)** and **Total eIF2 α** in the cell lysate. Data can be expressed as either the signal at 665 nm or the 665 nm/615 nm ratio.

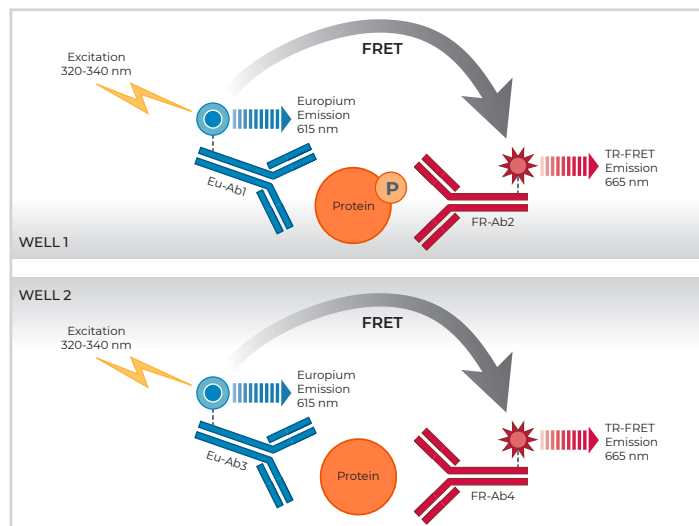


Fig. 1 Schematic representation of the TR-FRET cell signaling assay principle.

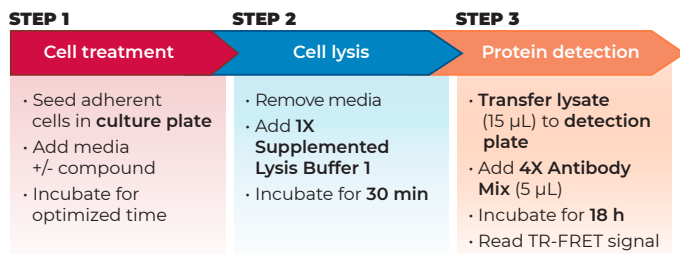


Figure 2 Assay workflow using the 2-plate (transfer) protocol.

KIT COMPONENTS

	500 points*
Eu-labeled phospho-eIF2 α (S51) antibody (Eu-Ab1)	20 μ L
Acceptor-labeled phospho-eIF2 α (S51) antibody (FR-Ab2)	80 μ L
Eu-labeled total-eIF2 α antibody (Eu-Ab3)	5 μ L
Acceptor-labeled total-eIF2 α antibody (FR-Ab4)	20 μ L
Lysis Buffer 1 (5X)	5 mL
Detection Buffer (10X)	250 μ L
Positive control cell lysate	500 μ L

* The number of assay points is based on an assay volume of 20 μ L in half-area 96-well or low-volume 384-well assay plates using the kit components at the recommended concentrations (refer to the User Manual).

TECHNICAL DATA SHEET

Phospho-eIF2 α (S51) + Total eIF2 α

VALIDATION DATA


This assay kit has been validated for the relative quantification of phospho-eIF2 α (S51) and total eIF2 α in HeLa cell lysates using the 2-plate assay protocol.

- Adherent cells were cultured overnight in a 96-well tissue culture plate (DMEM +10% FBS).
- Following cell treatment, the media was removed and cells were lysed with the 1X **Lysis Buffer 1** (50 μ L) supplemented with the phosphatase inhibitors sodium fluoride (1 mM) and sodium orthovanadate (2 mM).
- Following a **30-min** incubation at room temperature (RT) on an orbital shaker (400 rpm), lysates (15 μ L) were then transferred

to a 384-well assay plate followed by addition to separate wells of either the labeled antibodies Eu-Ab1 and FR-Ab2 (5 μ L) for detection of phospho-eIF2 α (S51) or Eu-Ab3 and FR-Ab4 (5 μ L) for detection of total eIF2 α .


- The plate was incubated at RT for **18 hours** and the TR-FRET signal was recorded at 665 and 615 nm (EnVision[®]; lamp excitation).

STIMULATION OF PHOSPHO-eIF2 α (S51) IN HELA CELLS

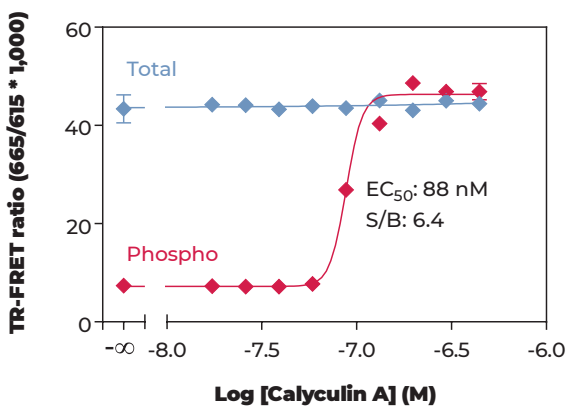


HeLa cells (20,000 cells/well; in triplicate) were incubated with serial dilutions Calyculin A for 30 min at RT. Data show that treatment of HeLa cells with Calyculin A stimulates phosphorylation of eIF2 α at S51 but does not affect the levels of total eIF2 α .

HELA CONTROL LYSATE TITRATION (QC TEST) PHOSPHO-eIF2 α (S51)

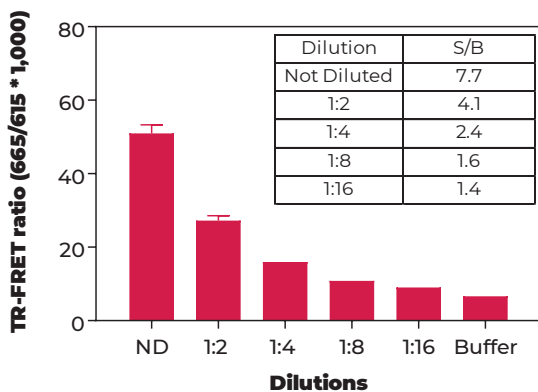

HELA CONTROL LYSATE TITRATION (QC TEST) TOTAL eIF2 α

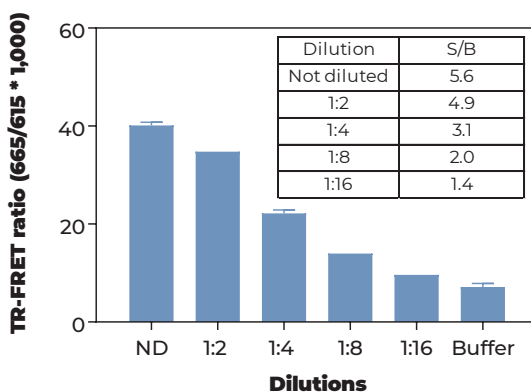

Quality Control: the Phospho-eIF2 α (S51) + Total eIF2 α assay kit is routinely tested against Calyculin A-treated HeLa lysates. HeLa cells were cultured in a 96-well tissue to 90% confluence and stimulated with 300 nM of Calyculin A for 30 min at RT. Following cell lysis using 50 μ L/well of 1X Lysis Buffer 1, lysates were serially diluted with 1X Lysis Buffer 1 and tested in triplicate and in separate wells for phospho-eIF2 α (S51) and total eIF2 α . Data show a linear relationship between lysate dilutions and TR-FRET ratio values.



bioauxilium

FOR MORE INFORMATION ON DEVELOPING AND OPTIMIZING TR-FRET CELL SIGNALING ASSAYS, CONSULT THE USER MANUAL.

7171 Frederick-Banting, Suite 2115, Montréal (Québec) H4S 1Z9 CANADA bioauxilium.com 1-866-610-6933 x 103