

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten! See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere Liefer- und Versandbedingungen

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

linkedin.com/company/szaboscandic in





6044 Cornerstone Court W, Ste E San Diego, CA 92121 **Tel:** 1.858.829.3082

Fax: 1.858.481.8694
Email: info@bpsbioscience.com

Data Sheet Hsp90α Assay Kit Catalog # 50298

Size: 384 reactions

DESCRIPTION: Hsp 90α is a molecular chaperone with essential functions in maintaining transformation. Inhibition of Hsp 90α function has been shown to play a role in tumorigenesis and disease progression. The *Hsp90\alpha Assay Kit* is designed for identification of Hsp 90α inhibitors using fluorescence polarization. The assay is based on the competition of fluorescently labeled geldanamycin, an HSP90 inhibitor, for binding to purified recombinant Hsp 90α .

The $Hsp90\alpha$ Assay Kit comes in a convenient 384-well format, with enough purified $Hsp90\alpha$ enzyme, FITC-labeled geldanamycin, and $Hsp90\alpha$ assay buffer for 400 enzyme reactions. The key to the $Hsp90\alpha$ Assay Kit is the fluorescently labeled geldanamycin. Using this kit, only one simple step on a microtiter plate is required for $Hsp90\alpha$ reactions. The FITC-labeled geldanamycin is incubated with a sample containing $Hsp90\alpha$ enzyme to produce a change in fluorescent polarization that can then be measured using a fluorescence reader.

COMPONENTS:

Catalog #	Component	Amount	Storage	
50290	Hsp90α recombinant enzyme	140 µg	-80°C	Avoid
50312	FITC-labeled geldanamycin (2.5 μM)	2 x 30 µl	-80°C	freeze/
50311	5x Hsp90 Assay Buffer 1	2 x 4 ml	-20°C	thaw
	Black, low binding NUNC microtiter	1	Room	cycles!
	plate		temp.	cycles:

MATERIALS OR INSTRUMENTS REQUIRED BUT NOT SUPPLIED:

40 mM DTT

2 mg/ml BSA (bovine serum albumin)

APPLICATIONS: Great for studying enzyme kinetics and screening small molecular inhibitors for drug discovery and HTS applications.

STABILITY: Up to 1 year when stored as recommended.

REFERENCES:

- 1. Kim J, et al., Biomol. Screening 2004; **9(5)**: 375-381.
- 2. Howes R, et al., Anal. Biochem. 2006; 350:202-213.



6044 Cornerstone Court W, Ste E San Diego, CA 92121

Tel: 1.858.829.3082 Fax: 1.858.481.8694 Email: info@bpsbioscience.com

ASSAY PROTOCOL:

Immediately prior to assay:

- 1) Thaw **FITC-labeled geldanamycin** on ice. Upon first thaw, briefly spin tube containing FITC-labeled geldanamycin to recover full content of the tube. Aliquot into single use aliquots. Store remaining FITC-labeled geldanamycin in aliquots at -80°C immediately. *Note: FITC-labeled geldanamycin is very sensitive to freeze/thaw cycles. Avoid multiple freeze/thaw cycles.*
- 2) Thaw **Hsp90**α on ice. Upon first thaw, briefly spin tube containing Hsp90α to recover full content of the tube. Aliquot Hsp90α into single use aliquots. Store remaining Hsp90α in aliquots at -80°C immediately. *Note:* Hsp90α is very sensitive to freeze/thaw cycles. Avoid multiple freeze/thaw cycles.

Step 1:

All samples and controls should be tested in duplicate.

- 1) Dilute FITC-labeled geldanamycin (2.5 μM stock) 25-fold with 1x Hsp90 assay buffer to make a 100 nM solution. (Make only sufficient quantity needed for the assay; store remaining 2.5 μM stock solution in aliquots at -80°C.)
- 2) Dilute Hsp90α in 1x Hsp90 assay buffer to 35 ng/μl (350 ng/reaction)*. Aliquot any remaining enzyme and store undiluted at -80°C. Keep diluted enzyme on ice. Discard any remaining diluted enzyme after use. *Note: optimal enzyme concentration may vary with the specific activity of the enzyme.
- 3) Prepare the master mixture: N wells x (7.5 μ l **5x Hsp90 assay buffer 1** + 2.5 μ l **40 mM DTT** + 2.5 μ l **2 mg/ml BSA** + 20 μ l **H₂O**). Add 32.5 μ l of master mixture to all wells.

	Blank	Enzyme Positive Control	Enzyme Negative Control	Test Inhibitor
5x Hsp90 assay buffer 1	7.5 µl	7.5 µl	7.5 µl	7.5 µl
40 mM DTT	2.5 µl	2.5 µl	2.5 µl	2.5 µl
2 mg/ml BSA	2.5 µl	2.5 µl	2.5 µl	2.5 µl
H ₂ O	20 µl	20 µl	20 µl	20 µl
FITC-Labeled geldanamycin (100 nM)	_	2.5 µl	2.5 µl	2.5 µl
Inhibitor	_	_	_	5 µl
Inhibitor Buffer (no inhibitor)	5 µl	5 µl	5 µl	_
1x HSP90 assay buffer	12.5 µl	_	10 µl	_
Hsp90α (35 ng/μl)	_	10 µl	_	10 µl
Total	50 μl	50 μl	50 μl	50 μl



6044 Cornerstone Court W, Ste E San Diego, CA 92121

Tel: 1.858.829.3082 Fax: 1.858.481.8694 Email: info@bpsbioscience.com

- 4) Add 2.5 μl of diluted FITC-labeled geldanamycin (100 nM) to each well designated "Enzyme Positive Control", "Enzyme Negative Control", and "Test Inhibitor."
- 5) Add 5 µl of **Inhibitor** to each well designated "Test Inhibitor." For the, "Blank", "Enzyme Positive Control" and "Enzyme Negative Control", add 5 µl of the same solution without Inhibitor (**Inhibitor Buffer**).
- 6) Add 10 μl of **1x HSP90 assay buffer** to the wells designated "Enzyme Negative Control". Add 12.5 μl **1x Hsp90 assay buffer** to the wells designated "Blank".
- 7) Initiate reaction by adding 10 μl of **diluted Hsp90**α (35 ng/μl), prepared as described above, to each well designated "Enzyme Positive Control" and "Test Inhibitor." Incubate at room temperature for 2 3 hours with slow shaking.

Step 2:

Read fluorescent polarization of the sample in a microtiter-plate reader capable of excitation at wavelengths ranging from 475-495 nm and detection of emitted light ranging from 518-538 nm. Blank value is subtracted from all other values.

CALCULATING RESULTS:

Definition of Fluorescence Polarization:

$$P = \frac{I_{II} - I_{\perp}}{I_{II} + I_{\perp}}$$

Where I_{\parallel} = Intensity with polarizers parallel and I_{\perp} = Intensity with polarizers perpendicular. Most instruments display fluorescence polarization in units of mP.

$$mP = \left(\frac{I_{II} - I_{\perp}}{I_{II} + I_{\perp}}\right) x \ 1000$$

The equation above assumes that light is transmitted equally well through both parallel and perpendicular oriented polarizers. In practice, this is generally not true and a correction must be made to measure the absolute polarization state of the molecule. This correction factor is called the "G Factor".



6044 Cornerstone Court W, Ste E San Diego, CA 92121

Tel: 1.858.829.3082 **Fax:** 1.858.481.8694


Email: info@bpsbioscience.com

$$mP = \left(\frac{I_{II} - G(I_{\perp})}{I_{II} + G(I_{\perp})}\right) x \ 1000$$
 OR $mP = \left(\frac{G(I_{II}) - I_{\perp}}{G(I_{II}) + I_{\perp}}\right) x \ 1000$

The G-factor is instrument-dependent and may vary slightly depending upon instrument and conditions. Please check the manual of your instrument to obtain the information about the establishment of the G-factor.

EXAMPLE OF ASSAY RESULTS

Hsp90 α activity (FITC-geldanamycin binding)

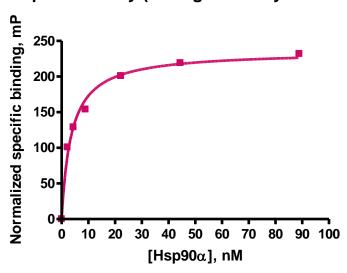

Binding of FITC-geldanamycin to HSP90α, measured using the Hsp90α Assay Kit, BPS Bioscience # 50298. Fluorescence was measured at λex 485nm, λem 530 nm using a Bio-Tek fluorescent microplate reader. *Data shown is lot-specific. For lot-specific information, please contact BPS Bioscience, Inc. at info@bpsbioscience.com*

RELATED PRODUCTS:

<u>Product</u>	<u>Cat. #</u>	<u>Size</u>
Hsp90α recombinant enzyme	50290	200 µg
Hsp90β recombinant enzyme	50292	200 µg
Aha1 recombinant enzyme	50291	200 µg
Geldanamycin inhibitor	27008	5 mg
MS-275 (Entinostat) inhibitor	27011	25 mg
Hsp90α Assay Kit (96 well)	50293	96 rxns
Hsp90β Assay Kit (96 well)	50294	96 rxns
Hsp90β Assay Kit (384 well)	50299	384 rxns