



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com


www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Data Sheet
PDE10A Assay Kit
 Catalog # 60400

DESCRIPTION: Phosphodiesterases (PDEs) play an important role in dynamic regulation of cAMP and cGMP signaling. PDE10A is a dual substrate PDE highly expressed in striatal medium spiny neurons. PDE10A inhibitors can improve the cognitive symptoms of schizophrenia, and exhibit potential therapeutic value for Huntington's Disease. The PDE10A Assay Kit is designed for identification of PDE10A inhibitors using fluorescence polarization. The assay is based on the binding of a fluorescent nucleotide monophosphate generated by PDE10A to the binding agent.

Phosphodiesterases catalyze the hydrolysis of the phosphodiester bond in dye-labeled cyclic monophosphates. Beads selectively bind the phosphate group in the nucleotide product. This increases the size of the nucleotide relative to unreacted cyclic monophosphate. In the polarization assay, dye molecules with absorption transition vectors parallel to the linearly-polarized excitation light are selectively excited. Dyes attached to the rapidly-rotating cyclic monophosphates will obtain random orientations and emit light with low polarization. Dyes attached to the slowly-rotating nucleotide-bead complexes will not have time to reorient and therefore will emit highly polarized light.

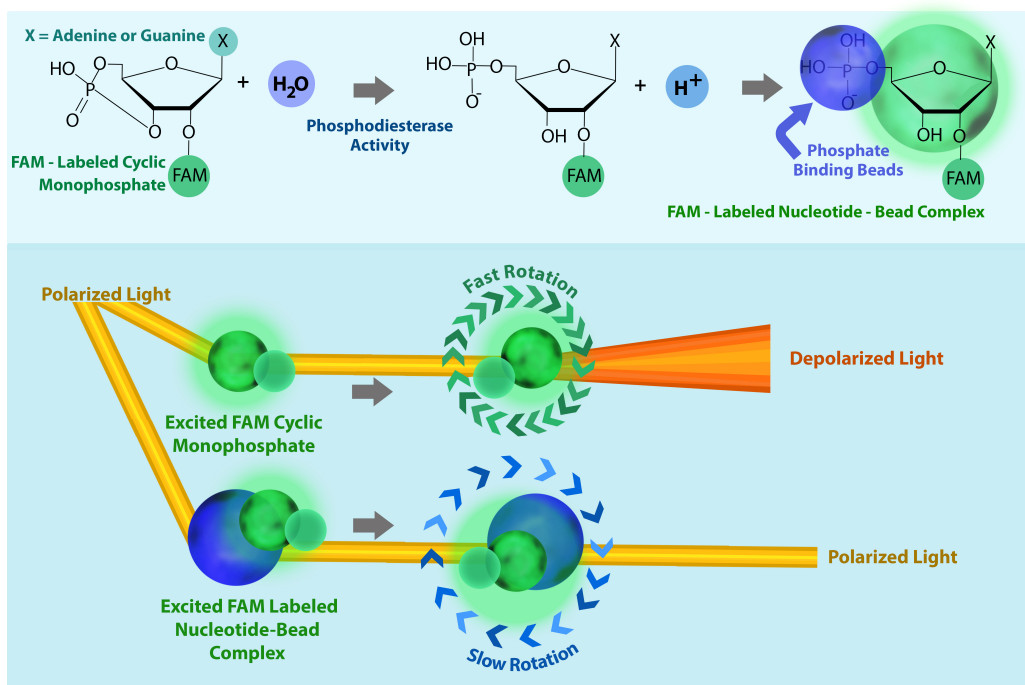

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Ct. West, Ste. B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

The PDE10A inhibitor screening assay kit comes in a convenient 96-well format, including purified PDE10A enzyme, fluorescently labeled PDE10A substrate (cAMP), binding agent, and PDE assay buffer for 100 enzyme reactions. The key to the PDE10A Assay Kit is the specific binding agent. Using this kit, only two simple steps on a microtiter plate are required for PDE10A reactions. First, the fluorescently labeled cAMP is incubated with a sample containing PDE10A for 1 hour. Second, a binding agent is added to the reaction mix to produce a change in fluorescent polarization that can then be measured using a fluorescence reader equipped for the measurement of fluorescence polarization.

COMPONENTS:

Catalog #	Component	Amount	Storage	
60100	PDE10A2 recombinant enzyme	>1 µg	-80°C	(Avoid freeze/ thaw cycles!)
60200	FAM-Cyclic-3', 5'-AMP: 20 µM	50 µl	-80°C	
60393	PDE Assay Buffer	25 ml	-20°C	
60390	Binding Agent	100 µl	+4°C	
60391	Binding Agent Diluent (cAMP)	10 ml	+4°C	
79685	Black, low binding, microtiter plate	1	Room temp.	

MATERIALS OR INSTRUMENTS REQUIRED BUT NOT SUPPLIED:

Fluorescent microplate reader capable of measuring fluorescence polarization

APPLICATIONS: Great for studying enzyme kinetics and screening small molecular inhibitors for drug discovery and HTS applications.

STABILITY: 6 months from date of receipt when stored as directed

REFERENCES:

1. Threlfall S, et al. (2009) *Pharmacol Exp Ther* **328(3)**:785-95.
2. Menniti FS, et al. (2007) *Curr Opin Investig Drugs* **8(1)**:54-9.

ASSAY PROTOCOL:

All samples and controls should be tested in duplicate.

Step 1:

- 1) Dilute **cAMP 20 µM** stock 100-fold with **PDE Assay Buffer** to make a 200 nM solution. Make only sufficient quantity needed for the assay; store remaining 20 µM stock solution in aliquots at -20°C.
- 2) Add 25 µl of **FAM-Cyclic-3',5'-AMP** (200 nM) to each well designated "Substrate Control", "Positive Control", and "Test Inhibitor". Add 25 µl of **PDE Assay Buffer** to each well designated "Blank".

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Ct. West, Ste. B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

- 3) Add 5 μ l of inhibitor solution to each well designated "Test Inhibitor". Add 5 μ l of the same solution without inhibitor (inhibitor buffer) to the "Blank", "Substrate Control" and "Positive Control".
- 4) Add 20 μ l of **PDE Assay Buffer** to the wells designated as the "Blank" and "Substrate Control".
- 5) Thaw **PDE10A** on ice. Upon first thaw, briefly spin tube containing enzyme to recover the full contents of the tube. Aliquot **PDE10A** enzyme into single-use aliquots. Store remaining undiluted enzyme in aliquots at -80°C immediately. *Note: **PDE10A** is very sensitive to freeze/thaw cycles. Do not re-use thawed aliquots or diluted enzyme.*
- 6) Dilute **PDE10A** to 10-20 pg/ μ l (200-400 pg/reaction) in **PDE Assay Buffer***. Initiate reaction by adding 20 μ l of diluted **PDE10A** to the wells designated for the "Positive Control" and "Test Inhibitor". Discard any remaining diluted enzyme after use. **Note: optimal enzyme concentration may vary with the specific activity of the enzyme.*
- 7) Incubate at room temperature for 1 hour.

	Blank	Substrate Control	Positive Control	Test Inhibitor
FAM-Cyclic-3',5'-AMP (200 nM)	-	25 μ l	25 μ l	25 μ l
PDE assay buffer	45 μ l	20 μ l	-	-
Test Inhibitor	-	-	-	5 μ l
Inhibitor Buffer (no inhibitor)	5 μ l	5 μ l	5 μ l	-
PDE10A2 (10-20 pg/ μ l)	-	-	20 μ l	20 μ l
Total	50 μl	50 μl	50 μl	50 μl

Step 2:

- 1) Shake the tube containing the binding agent to ensure it is thoroughly mixed. Mix **binding agent** thoroughly and dilute **binding agent** 1:100 with binding agent diluent.
- 2) Add 100 μ l diluted binding agent to each microwell. Incubate at room temperature for 1 hour with slow shaking.
- 3) Read the fluorescent polarization of the sample in a microtiter-plate reader capable of excitation at wavelengths ranging from 485 ± 5 nm and detection of emitted light ranging from 528 ± 5 nm. Blank value is subtracted from all other values.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Ct. West, Ste. B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

CALCULATING RESULTS:

Definition of Fluorescence Polarization:

$$P = \frac{I_{\parallel} - I_{\perp}}{I_{\parallel} + I_{\perp}}$$

where I_{\parallel} = Intensity with polarizers parallel and I_{\perp} = Intensity with polarizers perpendicular.

The equation above assumes that light is transmitted equally well through both parallel and perpendicular oriented polarizers. In practice, this is generally not true and a correction must be made to measure the absolute polarization state of the molecule. This correction factor is called the "G Factor".

$$FP(\text{measured}) = \frac{(I_{\parallel} - G \cdot I_{\perp})}{(I_{\parallel} + G \cdot I_{\perp})} * 1000$$

The G-factor is instrument-dependent and may vary slightly depending upon instrument and conditions. Please check the manual of your instrument to obtain the information about the establishment of the G-factor.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**


Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com

EXAMPLE OF ASSAY RESULTS:

PDE10A2 Activity

Substrate Conc. = 100nM (cAMP)

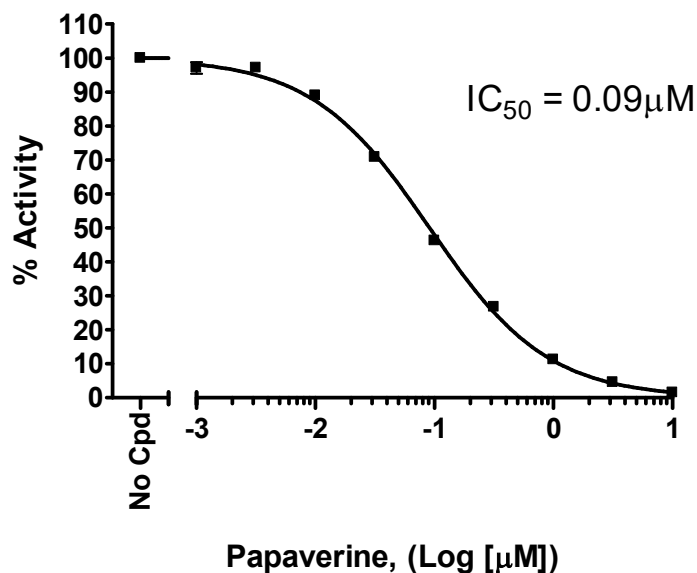

Inhibition of PDE10A2 by Papaverine, measured using the PDE10A Assay Kit, Cat. #60400. Fluorescence polarization was measured at 528 nm using a Tecan M1000 fluorescent microplate reader. *Data shown is lot-specific. For lot-specific information, please contact BPS Bioscience, Inc. at info@bpsbioscience.com*

RELATED PRODUCTS:

Product	Cat. #	Size
PDE10A1	60099	10 µg
PDE10A2	60100	10 µg
PDE10A (mouse)	60101	10 µg
PDE10A (rat)	60102	5 µg
PDE Assay Kit	60300	96 rxns.
PDE1B Assay Kit	60311	96 rxns.
PDE2A Assay Kit	60320	96 rxns.
PDE4A Assay Kit	60340	96 rxns.
PDE4D Assay Kit	60345	96 rxns.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com