



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com


www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Data Sheet **PDE3A Assay Kit** Catalog #79736

DESCRIPTION: Phosphodiesterases (PDEs) play an important role in dynamic regulation of cAMP and cGMP signaling. PDE3A, also known as cGMP-inhibited phosphodiesterase, has been implicated in cardiovascular function and fertility. The *PDE3A Assay Kit* is designed for identification of PDE3A inhibitors using fluorescence polarization. The assay is based on the binding of a fluorescent nucleotide monophosphate generated by PDE3A to the binding agent.

Phosphodiesterases catalyze the hydrolysis of the phosphodiester bond in dye-labeled cyclic monophosphates. Beads selectively bind the phosphate group in the nucleotide product. This increases the size of the nucleotide relative to unreacted cyclic monophosphate. In the polarization assay, dye molecules with absorption transition vectors parallel to the linearly-polarized excitation light are selectively excited. Dyes attached to the rapidly-rotating cyclic monophosphates will obtain random orientations and emit light with low polarization. Dyes attached to the slowly-rotating nucleotide-bead complexes will not have time to reorient and therefore will emit highly polarized light.

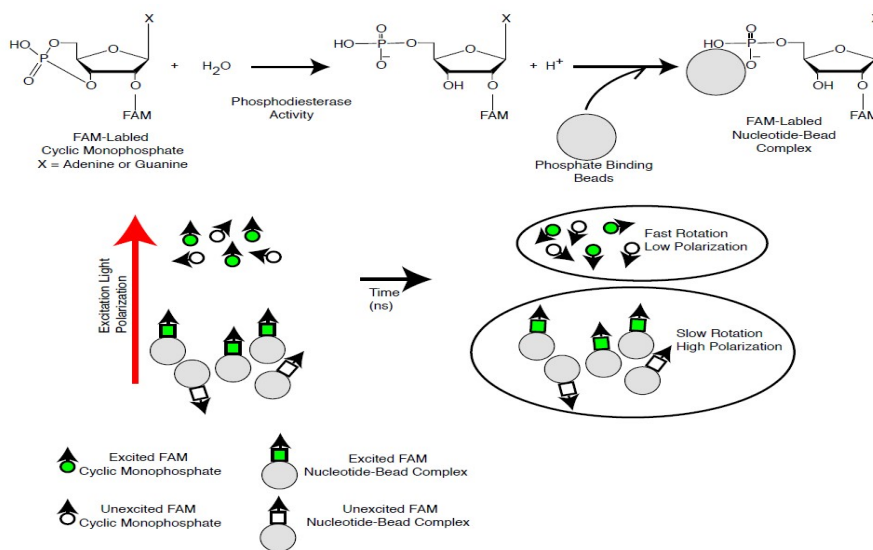

The PDE3A inhibitor screening assay kit comes in a convenient 96-well format, with purified human PDE3A enzyme, fluorescently labeled PDE3 substrate (cAMP), binding agent, and PDE assay buffer for 100 enzyme reactions. The key to the *PDE3A Assay Kit* is the specific binding agent. Using this kit, only two simple steps on a microtiter plate are required for PDE3A reactions. First, the fluorescently labeled cAMP is incubated with a sample containing PDE3A

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
 Or you can Email us at: info@bpsbioscience.com
 Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

for 1 hour. Second, binding agent is added to the reaction mix to produce a change in fluorescent polarization that can then be measured using a fluorescence reader equipped for the measurement of fluorescence polarization.

COMPONENTS:

Catalog #	Component	Amount	Storage	
60032	PDE3A recombinant enzyme	>1 µg	-80°C	(Avoid freeze/thaw cycles!)
60200	FAM-Cyclic-3', 5'-AMP (20 µM)	50 µl	-80°C	
60393	PDE assay buffer	25 ml	-20°C	
60390	Binding Agent	100 µl	+4°C	
60391	Binding Agent Diluent	10 ml	+4°C	
79685	Black, low binding, microtiter plate	1	Room temp.	

MATERIALS OR INSTRUMENTS REQUIRED BUT NOT SUPPLIED:

Fluorescent microplate reader capable of measuring fluorescence polarization
Adjustable micropipettor and sterile tips.
1,4-Dithiothreitol (DTT) 1 M in anhydrous DMSO.

APPLICATIONS: Great for studying enzyme kinetics and screening small molecular inhibitors for drug discovery and HTS applications.

STABILITY: 6 months from date of receipt when stored as directed.

REFERENCE: Maurice DH. *Front. Biosci.* 2005; **10**:1221-8.

ASSAY PROTOCOL:

All samples and controls should be tested in duplicate.

Step 1:

- 1) Dilute 20 µM **FAM-Cyclic-3', 5'-AMP** stock 100-fold with **PDE assay buffer** to make a 200 nM solution. Make only sufficient quantity needed for the assay; store remaining 20 µM stock solution in aliquots at -20°C.
- 2) Dilute 1M 1,4-Dithiothreitol (DTT) 1:500 into the diluted **FAM-Cyclic-3',5'-AMP**. For example, add 10 µl DTT (1M) to 5 ml of diluted FAM-Cyclic-3', 5'-AMP (200 nM).
- 3) Add 25 µl of **FAM-Cyclic-3',5'-AMP** (200 nM) to each well designated "Positive Control", "Test Inhibitor", and "Substrate Control".

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
Or you can Email us at: info@bpsbioscience.com
Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

- 4) Add 20 μ l of **PDE assay buffer** to each well designated "Substrate Control" and 45 μ l of **PDE assay buffer** to each well designated "Blank".
- 5) Add 5 μ l of inhibitor solution to each well designated "Test Inhibitor". For the wells labeled "Positive Control", "Substrate Control" and "Blank", add 5 μ l of the same solution without inhibitor (**PDE assay buffer**).
- 6) Thaw **PDE3A** on ice. Upon first thaw, briefly spin tube containing enzyme to recover the full contents of the tube. Aliquot **PDE3A** enzyme into single-use aliquots. Store remaining undiluted enzyme in aliquots at -70°C immediately. *Note: PDE3A is very sensitive to freeze/thaw cycles. Do not re-use thawed aliquots or diluted enzyme.*
- 7) Dilute **PDE3A** in **PDE assay buffer** to 2.5 pg/ μ l (0.05 ng/reaction)*. Initiate reaction by adding 20 μ l of diluted **PDE3A** to the wells designated "Positive Control" and "Test Inhibitor." Discard any remaining diluted enzyme after use. **Note: Optimal enzyme concentration may vary with the specific activity of the enzyme.*
- 8) Incubate at room temperature for 1 hour.

	Positive Control	Test Inhibitor	Substrate Control	"Blank" Negative Control
FAM-Cyclic-3',5'-AMP (200 nM)	25 μ l	25 μ l	25 μ l	-
PDE assay buffer	-	-	20 μ l	45 μ l
Inhibitor (in PDE assay buffer)	-	5 μ l	-	-
PDE assay buffer (no inhibitor)	5 μ l	-	5 μ l	5 μ l
PDE3A (2.5 pg/ μ l)	20 μ l	20 μ l	-	-
Total	50 μl	50 μl	50 μl	50 μl

Step 2:

- 1) Mix **binding agent** thoroughly and dilute **binding agent** 1:100 with binding agent diluent.
- 2) Add 100 μ l diluted binding agent to each microwell. Incubate at room temperature for 1 hour with slow shaking.

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
Or you can Email us at: info@bpsbioscience.com
Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

- 3) Read the fluorescent polarization of the sample in a microtiter-plate reader equipped for the measurement of fluorescence polarization, capable of excitation at wavelengths ranging from 485 ± 5 nm and detection of emitted light ranging from 528 ± 10 nm. Blank value is subtracted from all other values.

CALCULATING RESULTS:

Definition of Fluorescence Polarization:

$$P = \frac{I_{\parallel} - I_{\perp}}{I_{\parallel} + I_{\perp}}$$

where I_{\parallel} = Intensity with polarizers parallel and I_{\perp} = Intensity with polarizers perpendicular.

The equation above assumes that light is transmitted equally well through both parallel and perpendicular oriented polarizers. In practice, this is generally not true and a correction must be made to measure the absolute polarization state of the molecule. This correction factor is called the "G Factor".

$$FP(\text{measured}) = \frac{([I_{\parallel}] - G*[I_{\perp}])}{([I_{\parallel}] + G*[I_{\perp}])} * 1000$$

The G-factor is instrument-dependent and may vary slightly depending upon instrument and conditions. Please check the manual of your instrument to obtain the information about the establishment of the G-factor.


OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**
Or you can Email us at: info@bpsbioscience.com
Please visit our website at: www.bpsbioscience.com



6042 Cornerstone Court W, Ste B
San Diego, CA 92121
Tel: 1.858.202.1401
Fax: 1.858.481.8694
Email: info@bpsbioscience.com

EXAMPLE OF ASSAY RESULTS:

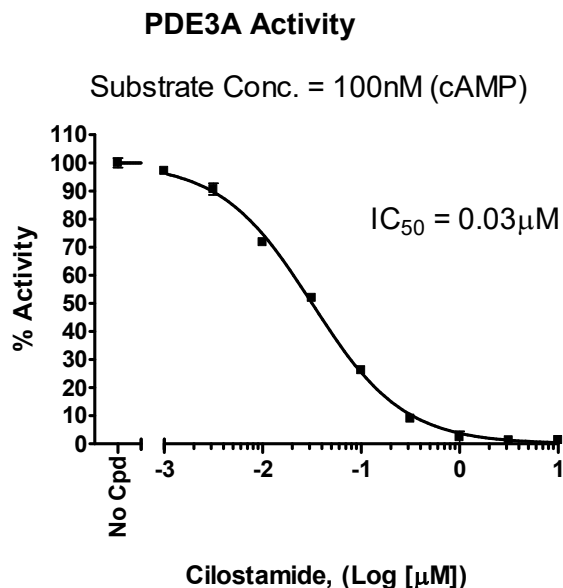

Inhibition of PDE3A by cilostamide, measured using the PDE3A Assay Kit, BPS Bioscience # 79736. Fluorescence polarization was measured at 528 nm using a Bio-Tek fluorescent microplate reader. *Data shown is lot-specific. For lot-specific information, please contact BPS Bioscience, Inc. at info@bpsbioscience.com*

RELATED PRODUCTS :

<u>Product</u>	<u>Cat. #</u>	<u>Size</u>
PDE3A	60030	10 µg
PDE3B	60031	10 µg
PDE3A (Mouse)	60036	5 µg
PDE3A (Dog)	100264	5 µg
PDE Assay Kit	60300	96 rxns.
PDE3A Assay Kit	60330	96 rxns.
PDE3B Assay Kit	60331	96 rxns.
PDE1B Assay Kit	60311	96 rxns.
PDE4A Assay Kit	60340	96 rxns.
PDE4D Assay Kit	60345	96 rxns.
PDE10A Assay Kit	60400	96 rxns.
FAM-cAMP Substrate	60200	100 nmol

OUR PRODUCTS ARE FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE.

To place your order, please contact us by Phone **1.858.202.1401** Fax **1.858.481.8694**

Or you can Email us at: info@bpsbioscience.com

Please visit our website at: www.bpsbioscience.com