



SZABO SCANDIC

Part of Europa Biosite

Produktinformation



Forschungsprodukte & Biochemikalien



Zellkultur & Verbrauchsmaterial



Diagnostik & molekulare Diagnostik



Laborgeräte & Service

Weitere Information auf den folgenden Seiten!
See the following pages for more information!



Lieferung & Zahlungsart

siehe unsere [Liefer- und Versandbedingungen](#)

Zuschläge

- Mindermengenzuschlag
- Trockeneiszuschlag
- Gefahrgutzuschlag
- Expressversand

SZABO-SCANDIC HandelsgmbH

Quellenstraße 110, A-1100 Wien

T. +43(0)1 489 3961-0

F. +43(0)1 489 3961-7

mail@szabo-scandic.com

www.szabo-scandic.com

[linkedin.com/company/szaboscandic](https://www.linkedin.com/company/szaboscandic) 

Anti-Human CD11a (TP1/40)

Fluorochrome	Reference	Test
PE	11APE-100T	100 test



PRODUCT DESCRIPTION

Other Names: Integrin alpha-L, CD11 antigen-like family member A, Leukocyte adhesion glycoprotein LFA-1 alpha chain, LFA-1A, Leukocyte function-associated molecule 1 alpha chain.

Description: The anti-CD11a monoclonal antibody derives from PMA and Ionomycin activated T cells blast (Human).

Clone: TP1/40

Isotype: Mouse IgG1, kappa

Reactivity: Human

Source: Supernatant proceeding from an in vitro cell culture of a cell hybridoma.

Purification: Affinity chromatography.

Composition: Mouse anti-human CD11a monoclonal antibody conjugated with a fluorochrome and in an aqueous solution which contains stabilising protein and 0.09% sodium azide (NaN₃).

Fluorochrome	Reagent provided	Concentration (µg/ml)
PE (R-Phycoerythrin)	25 ug in 2 ml	12,5

RECOMMENDED USAGE

Immunostep's CD11a, clone TP1/40, is a monoclonal antibody intended for *in vitro* diagnostic use in the identification and enumeration of human sample lymphocytes that express CD11a using flow cytometry.

CLINICAL RELEVANCE

This antibody can be used in flow cytometry for analysis of blood samples and bone marrow or immunohistochemistry. The CD11a antigen is expressed in human leucocytes. The monoclonal antibody is directed against the CD11a- antigen, located on the alpha-L chain of LFA-1 complex (Lymphocyte Function-associated Antigen-1), which is expressed on mature immunocompetent lymphocytes and their neoplastic counterparts, all leukocytes including B and T lymphocytes, monocytes, macrophages, neutrophils, basophils, and eosinophils. As recognized function are intercellular adhesion and costimulation. Antibodies to CD11a/CD18 block T cell responses to antigen presenting cells (including the mixed lymphocyte reaction) T cell help to B cells, CTL- and NK-mediated killing, macrophage killing of tumor cells, and leukocyte endothelium adhesion/extravasation.⁽⁶⁻¹⁰⁾

PRINCIPLES OF THE TEST

The anti-CD11a monoclonal antibody binds to the surface of cells that express the CD11a antigen. To identify these cells, the sample is incubated with the antibody and is analysed by flow cytometry.

APPROPRIATE STORAGE AND HANDLING CONDITIONS

Store in the dark, refrigerated between 2 °C and 8 °C. DO NOT FREEZE. The antibody is stable until the expiry date stated on the vial label if kept at 2°C-8°C. Do not use after the date indicated.

Once the vial is open, the product is stable for 90 days.

EVIDENCE OF DETERIORATION

Reagents should not be used if any evidence of deterioration is observed. For more information, please contact our technical service: tech@immunostep.com

The product's normal appearance is a semi-transparent, colourless liquid. It should not be used if liquid medium is cloudy or contains precipitate. It should be odourless.

RECOMMENDATIONS AND WARNINGS

- The reagents contain sodium azide. In acid conditions, it is transformed into hydrazoic acid, a highly toxic compound. Azide compounds must be diluted in running water before being discarded. These conditions are recommended so as to avoid deposits in plumbing, where explosive conditions could develop. The safety data sheet (SDS) is available online at www.immunostep.com
- Avoid microbial contamination of the reagent.
- Protect from light. Use dim light during handling, incubation with cells and prior to analysis.
- Never mouth pipette.
- In the case of contact with skin, wash in plenty of water.
- The samples should be handled in the same way as those capable of transmitting infection. Appropriate handling procedures should be guaranteed.
- Do not use after the expiry date indicated on the vial.
- Deviations from the recommended procedure could invalidate the analysis results.
- FOR *IN VITRO* DIAGNOSTIC USE.
- For professional use only.
- Before acquiring the samples, it is necessary to make sure that the flow cytometer is calibrated and compensated.

SAMPLE COLLECTION

The extraction of venous blood samples should be carried out in blood collection tubes using the appropriate anticoagulant (EDTA or heparin)^(1,2,3). For optimum results, the sample should be processed during the six hours following the extraction. Samples which cannot be processed within the 48 hours following the extraction should be discarded.

MATERIALS REQUIRED BUT NOT PROVIDED

- Isotype controls:

Fluorochrome	Isotype control	Immunostep Reference
PE	Mouse IgG1	ICIGG1PE-50UG

- Centrifuge
- Commonly used 12 x 75-mm flow cytometry assay tubes
- Micropipettes for dispensing volumes from 5 µl to 2 ml
- Blood collection tubes with anticoagulant.
- Phosphate buffered saline (PBS) with 0.09% sodium azide. It is recommendable to add 0.5% BSA
- Vacuum system
- Lysing solution
- Flow cytometer equipped with laser and appropriate fluorochrome filters
- Vortex Agitator

SAMPLE PREPARATION:

1. Add the suggested volume indicated on the antibody vial to a 12x75-mm cytometer tube. It is advisable to prepare an additional tube with the appropriate isotype control (*please see materials required but not provided*).
2. Add 100 µL of sample (up to 10⁶ cells) and mix properly in the vortex.
3. Incubate in the dark for 15 minutes at room temperature (20-25°C) or for 30 minutes at 4°C.
4. Add 2 ml of the lysing solution, mix in the vortex and incubate in the dark for 10 minutes or until the sample is lysed.
5. Centrifuge at 540g for five minutes and carefully withdraw the supernatant by suction so as not to touch the cell pellet. Leave 50 µl of non-aspirated liquid.
6. Resuspend pellet.
7. Add 2 ml of PBS (*please see materials required but not provided*).
8. Centrifuge at 540g for five minutes and carefully withdraw the supernatant by suction so as not to touch the cell pellet. Leave 50 µl of non-aspirated liquid.
9. Resuspend the pellet in 0.3 ml of PBS.

Acquire on a flow cytometer or store in the dark at 2°C -8°C until the analysis is carried out. Samples should be acquired within the 3 hour after lysis.

FLOW CYTOMETRY ANALYSIS

Collect the fluorescence attributed to monoclonal antibody CD11a and determine the percentage of stained cells. It is necessary to use an isotope control conjugated with the same fluorochrome, of the same type of immunoglobulin heavy chain and concentration as that of the CD11a, so as to evaluate and correct the unspecific binding of lymphocytes (*please see materials required but not provided*). Set an analysis region to eliminate fluorescence background noise and to include positively stained cells.

Below is an example diagram of peripheral blood stained applying the protocol described in point 6:




Fig. 1: biparametric diagram of the average fluorescence intensity of the CD11a+ leucocyte population and its internal complexity (SSC) in a peripheral blood specimen from a healthy donor.

LIMITATIONS OF THE PROCEDURE

1. Incubation of antibody with cells for other than the recommended procedures may result in a reduction or loss of antigenic determinants from the cell surface.
2. The values obtained from normal individuals may vary from laboratory to laboratory; it is therefore suggested that each laboratory should establish its own normal reference range.
3. Abnormal cells or cell lines may show a higher antigen density than normal cells. In some cases, this could require the use of a greater quantity of monoclonal antibody than is indicated in the procedures for sample preparation.
4. In whole blood samples, red blood cells found in abnormal samples, as well as nucleated red cells (from both normal and abnormal specimens) may be resistant to lysis. Longer periods of red blood cell lysing may be needed in order to avoid the inclusion of unlysed cells in the lymphocyte gated region.
5. Blood samples should not be refrigerated for an extensive period (more than 24 hours), since the number of viable cells will gradually decrease, and this may have an effect on the analysis. In order to obtain the best values, they should be kept at room temperature immediately prior to incubation with the monoclonal antibody.
6. Accurate results with flow cytometric procedures depend on correct alignment and calibration of the lasers, as well as correct gate settings.

REFERENCE VALUES

Abnormal results in the percentage of cells expressing the antigen or in its levels of expression may be due to pathological conditions. It is advisable to know the normal antigen expression patterns in order to ensure a proper interpretation of the results^(4,5).

The values obtained from healthy individuals may vary from laboratory to laboratory; it is therefore suggested that each laboratory should establish its own normal reference range.

CHARACTERISTICS

SPECIFICITY

Blood samples were obtained from healthy normal donors of Caucasian were stained with Immunostep CD11a PE monoclonal antibody.

Cells contained in the lymphocyte, monocyte and granulocyte regions were selected for analysis. Blood samples were processed by a leukocyte method, with a direct immunofluorescence staining for flow cytometric analysis.

To evaluate the reagent's Specificity (cross-reactivity with other cell populations), 10 blood samples from healthy donors were studied, stained with an adequate isotype control and the MAb to study. The percentage of lymphocytes, monocytes and granulocytes stained with the mentioned MAb was evaluated. The results obtained are shown in the following table:

Case Summaries

	Lymphocytes	Monocytes	Granulocytes
1	99,60	100,00	100,00
2	99,78	100,00	100,00
3	99,29	100,00	100,00
4	99,33	100,00	100,00
5	99,28	100,00	100,00
6	98,74	100,00	100,00
7	97,04	100,00	100,00
8	92,82	100,00	100,00
9	95,36	100,00	100,00
10	99,11	100,00	100,00
Total N	10	10	10
Mean	98,0350	100,00	100,00
Median	99,1950	100,00	100,00
Minimum	92,82	100,00	100,00
Maximum	99,78	100,00	100,00
Desv. tip.	2,29228	,00000	,00000
Variance	5,255	,000	,000

SENSIBILITY

Sensitivity of the Immunostep CD11a monoclonal antibodies was determined by staining a blood sample from donor. Dilutions of a peripheral blood sample were made to check the concentration scale of stained cells obtained. The results show an excellent correlation level between the results obtained and expected based on the dilution used.

To determine the consistency of the conjugated monoclonal antibody as opposed to small variations (but deliberate). It provides an indication of its reliability during its normal use. The results are shown in the following table:


Case Summaries

	Sample	Dilution	% Expected	% Obtained
1	400A + 0B	100,0	47,31	47,31
2	350A + 50B	87,5	41,39	38,52
3	300A + 100B	75,0	35,48	32,87
4	250A + 150B	62,5	29,57	26,94
5	200A + 200B	50,0	23,65	22,64
6	150A + 250B	37,5	17,74	16,79
7	100A + 300B	25,0	11,82	11,04
8	50A + 350B	12,5	5,91	5,75
9	0A + 400B	,0	,00	,00
Total N	9	9	9	9

Model Summary

Modelo	R	R Square	Adjusted Square	Std. Error of the Estimate
1	,998 ^a	,996	,995	1,11101

a.Predictor: % Obtained

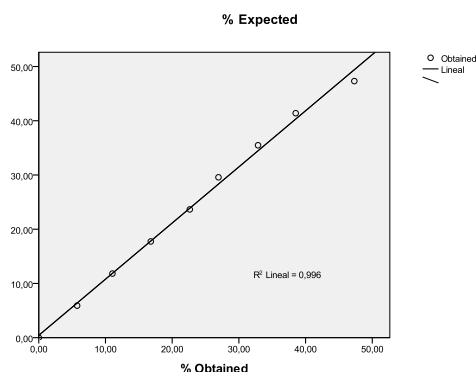

REPRODUCIBILITY

Reproducibility for the Immunostep CD11a: PE-conjugated monoclonal antibodies was determined by performing 10 replicated determinations of each antibody in each of three CD11a+ ranges, high, medium and low. Thus, a total of 30 determinations were performed for each form of CD11a. In this manner, reproducibility was demonstrated throughout the entire measuring range.

The 10 determinations for each range were performed by the staining, processing and analysis of 10 separate samples. Lymphocytes were selected for the analysis of percent cells stained in each of the three ranges.

To perform this study, anticoagulated blood was obtained from a normal donor expressing a high percentage of CD11a+ cells. Mid-range and low range samples were obtained by mixing known CD11a- cells in appropriate ratios, while maintaining the same total cell concentration for the three ranges.

The study was performed in each of three independent laboratories, in the manner that each laboratory obtained, stained and analyzed separate blood samples.

Case Summaries

	% High	% Medium	% Low
1	78,24	66,21	57,26
2	79,34	65,72	56,07
3	79,14	65,50	55,92
4	78,32	65,55	54,45
5	77,85	65,88	56,72
6	78,83	64,80	55,71
7	78,49	64,48	57,60
8	79,13	65,68	59,00
9	78,52	63,12	56,38
10	77,18	64,81	57,05
Total N	10	10	10

Descriptive Statistics

	% High	% Medium	% Low
N	10	10	10
Valid			
Missing	0	0	0
Mean	78,5040	65,1750	56,6160
Median	78,5050	65,5250	56,5500
Mode	77,18	63,12	54,45
Desv. tip.	,65712	,90348	1,23001
Variance	,432	,816	1,513
Range	2,16	3,09	4,55
Minimum	77,18	63,12	54,45
Maximum	79,34	66,21	59,00

*Note: Data analyzed with SPSS for Windows 17.0

WARRANTY

Warranted only to conform to the quantity and contents stated on the label or in the product labelling at the time of delivery to the customer. Immunostep disclaims hereby other warranties. Immunostep's sole liability is limited to either the replacement of the products or refund of the purchase price.

REFERENCES

1. Procedures for the collection of diagnostic blood specimens by venipuncture- approved standard; Fifth edition (2003). Wayne PA: National Committee for Clinical Laboratory Standards; Document H3-A5.
2. Standard Procedures for the Collection of Diagnostic Blood Specimens", publicado por el National Committee for Clinical Laboratory Standards (NCCLS)
3. Clinical applications of flow cytometry: Quality assurance and immunophenotyping of lymphocytes; approved guideline (1998). Wayne PA: National Committee for Clinical Laboratory Standards; Document H42-A.
4. Kotylo PK et al. Reference ranges for lymphocyte subsets in pediatric patients. Am J Clin Pathol 100:111-5 (1993)
5. Reichert et al. Lymphocyte subset reference ranges in adult Caucasians. Clin Immunol Immunopathol 60:190-208 (1991)
6. Sanchez-Madrid F, Krensky AM, Ware CF, Robbins E, Strominger JL, Burakoff SJ, et al. Three distinct antigens associated with human T-lymphocyte-mediated cytotoxicity: LFA-1, LFA-2, and LFA-3. Proc Natl Acad Sci U S A 1982 Dec;79(23):7489-93.
7. Sanchez-Madrid F, Nagy JA, Robbins E, Simon P, Springer TA. A human leukocyte differentiation antigen family with distinct alpha-subunits and a common beta-subunit: the lymphocyte function-associated antigen (LFA-1), the C3b complement receptor (CR3/CD11b), and the p150,95 molecule. J Exp Med 1983 Dec 1;158(6):1785-803.
8. Kishimoto TK, Hollander N, Roberts TM, Anderson DC, Springer TA. Heterogeneous mutations in the beta subunit common to the LFA-1, Mac-1, and p150,95 glycoproteins cause leukocyte adhesion deficiency. Cell 1987 Jul 17;50(2):193-202.
9. Springer TA, Dustin ML, Kishimoto TK, Marlin SD. The lymphocyte function-associated LFA-1, CD2, and LFA-3 molecules: cell adhesion receptors of the immune system. Annu Rev Immunol 1987;5:223-52.
10. Knapp W. Leucocyte typing IV: white cell differentiation antigens. Oxford: Oxford University Press; 1989.

MANUFACTURED BY



Immunostep S.L

Avda. Universidad de Coimbra, s/n
Cancer Research Center (CIC)
Campus Miguel de Unamuno
37007 Salamanca (Spain)
Tel. (+34) 923 294 827
www.immunostep.com